

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/02/2024

OPERATOR NAME:  
MAKENZIE A HAYES  
Permit #: 49532  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:51
INTERNAL STANDARD	VERIFIED	14:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:51
BLANK TEST	0.00	14:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:53
BLANK TEST	0.00	14:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:54
BLANK TEST	0.00	14:55

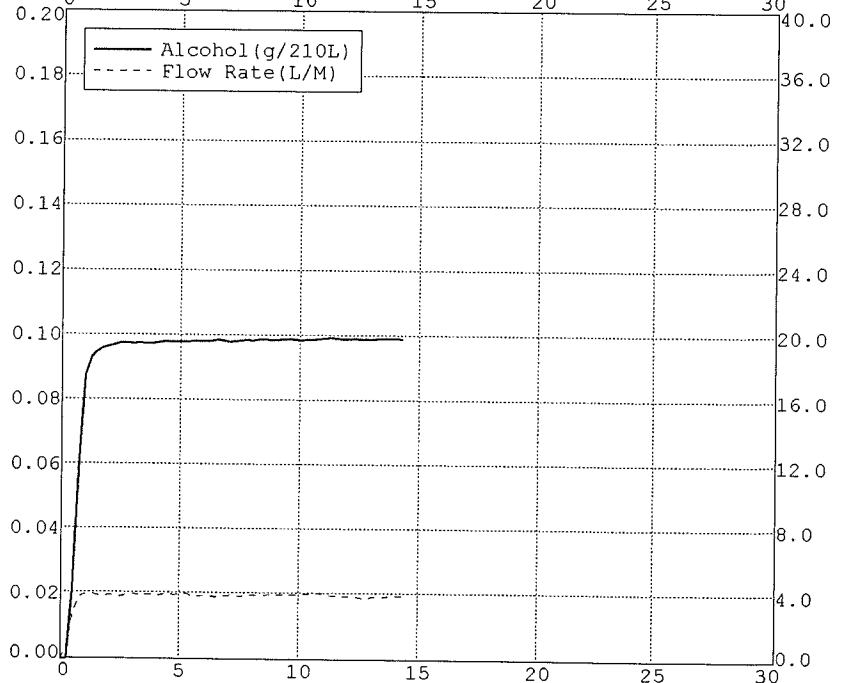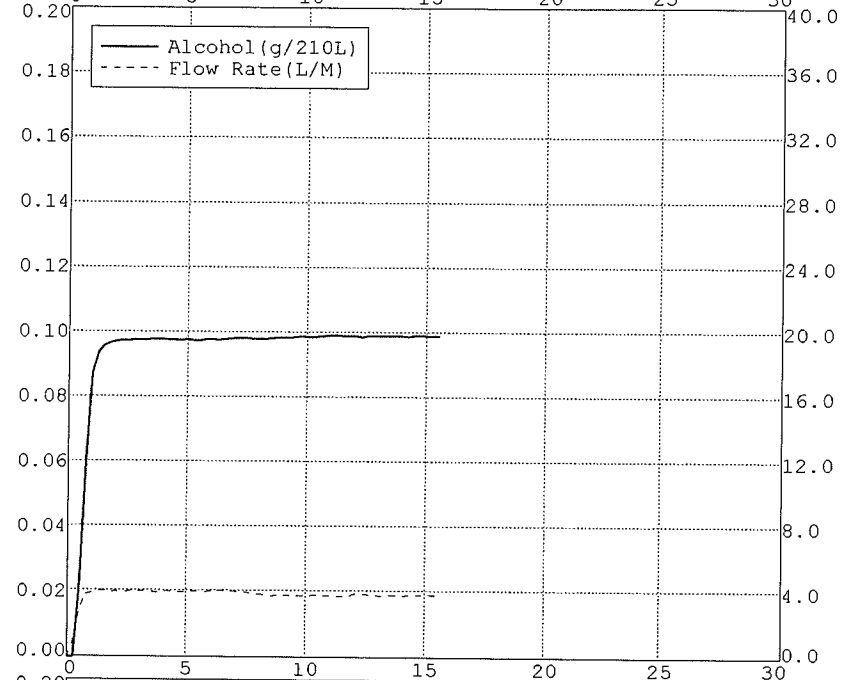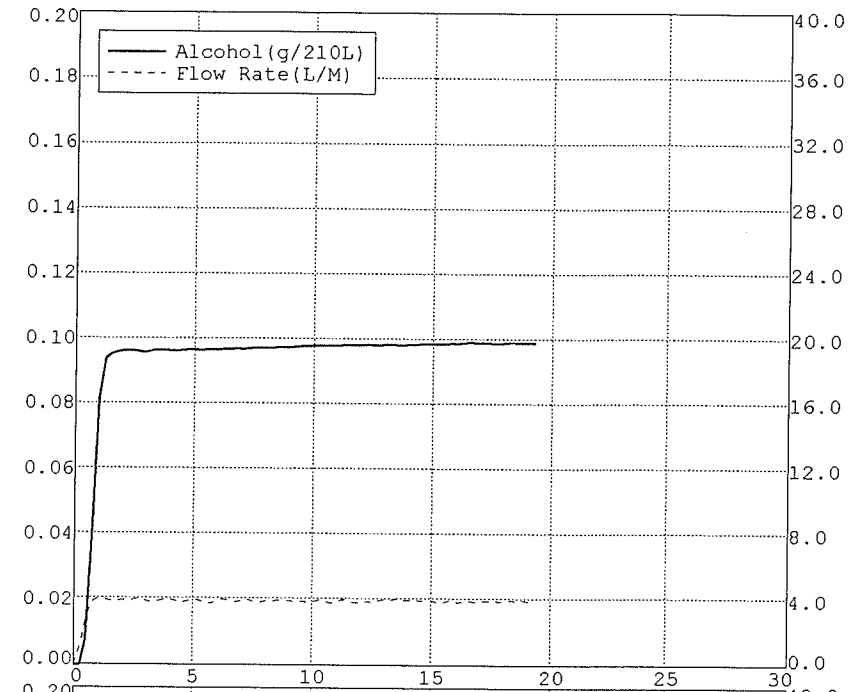

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/09/2024

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:28
INTERNAL STANDARD	VERIFIED	01:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:28
BLANK TEST	0.00	01:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:29
BLANK TEST	0.00	01:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:31
BLANK TEST	0.00	01:31

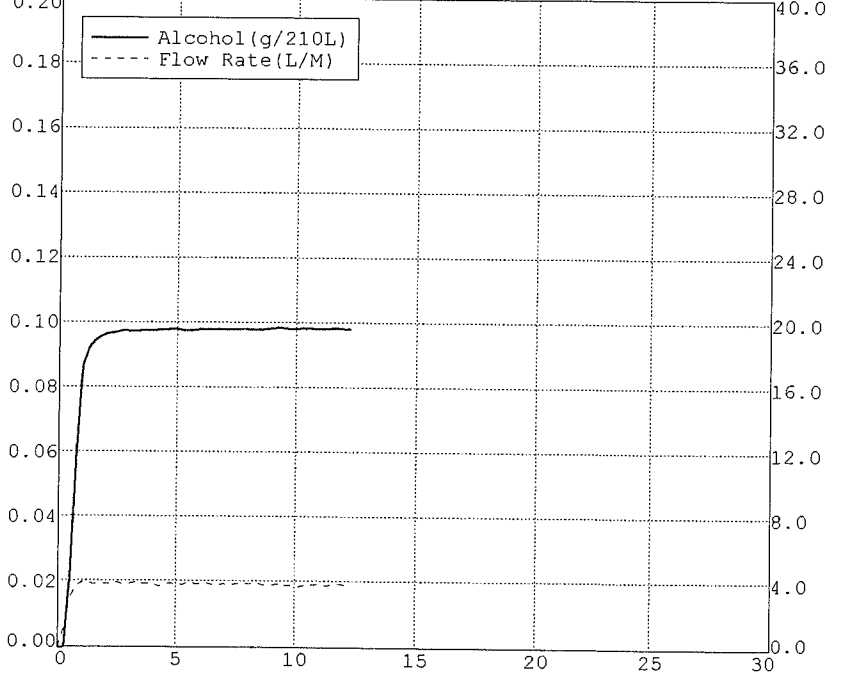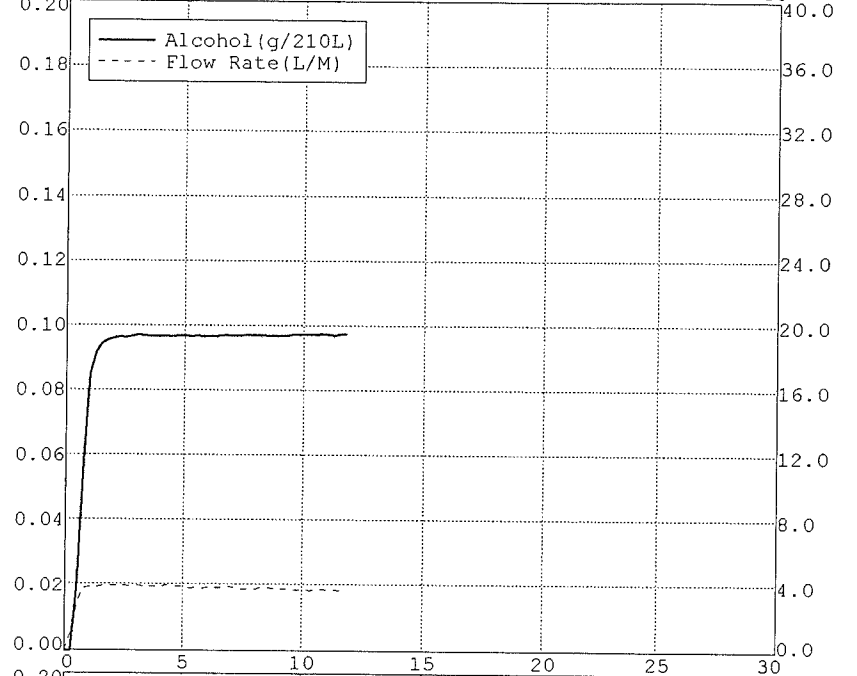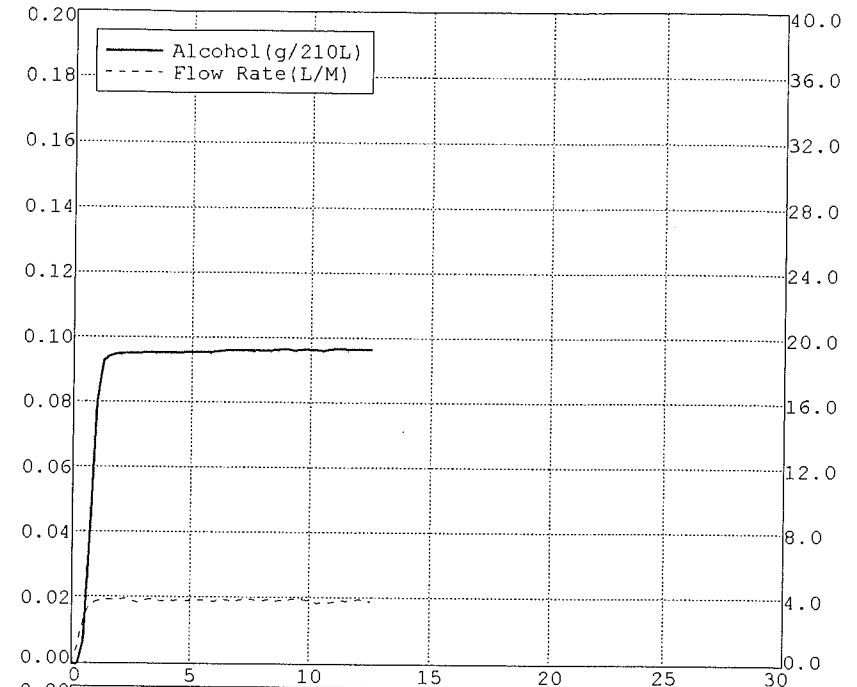

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/16/2024

OPERATOR NAME:  
MAKENZIE A HAYES  
Permit #: 49532  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:44
INTERNAL STANDARD	VERIFIED	18:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:45
BLANK TEST	0.00	18:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:46
BLANK TEST	0.00	18:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:47
BLANK TEST	0.00	18:48

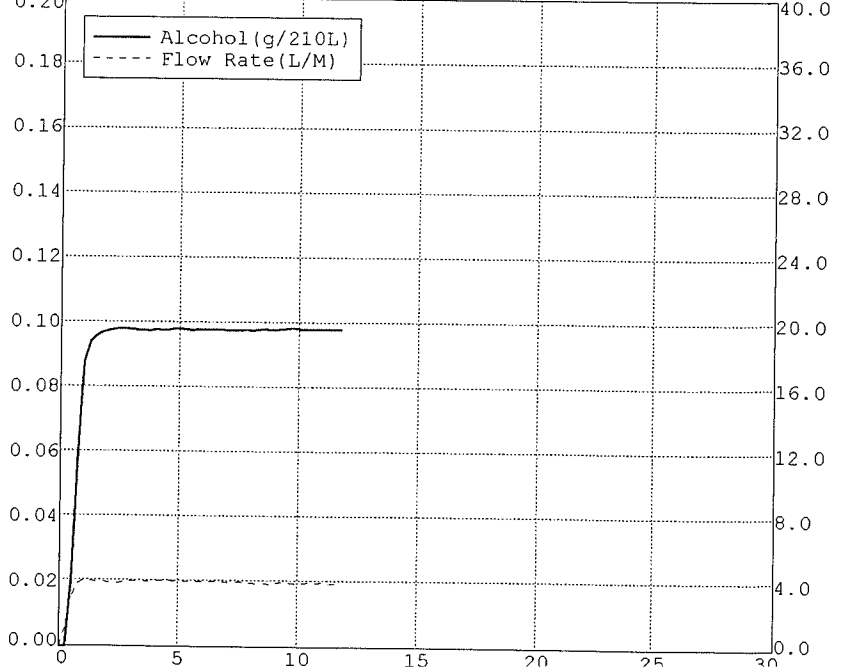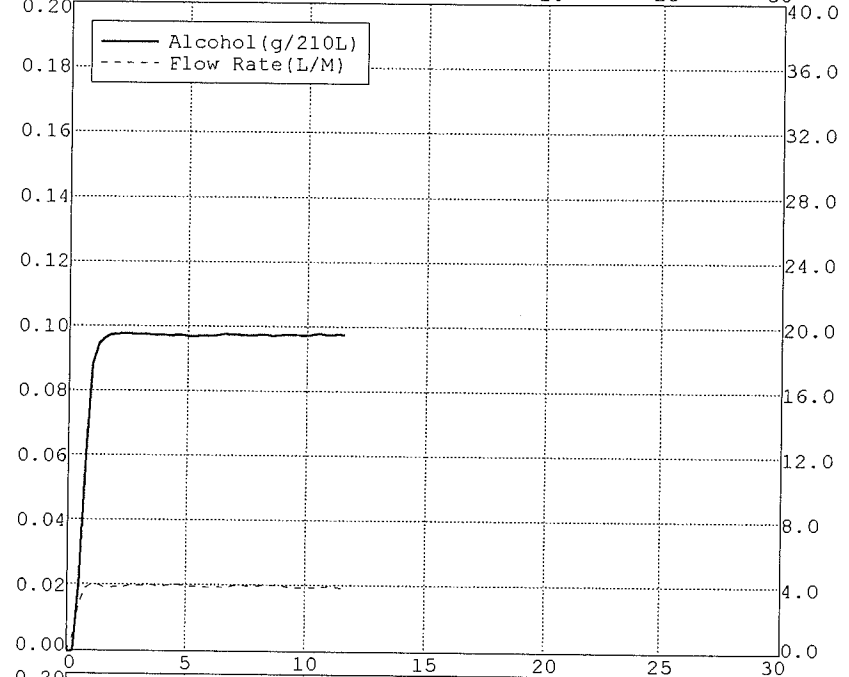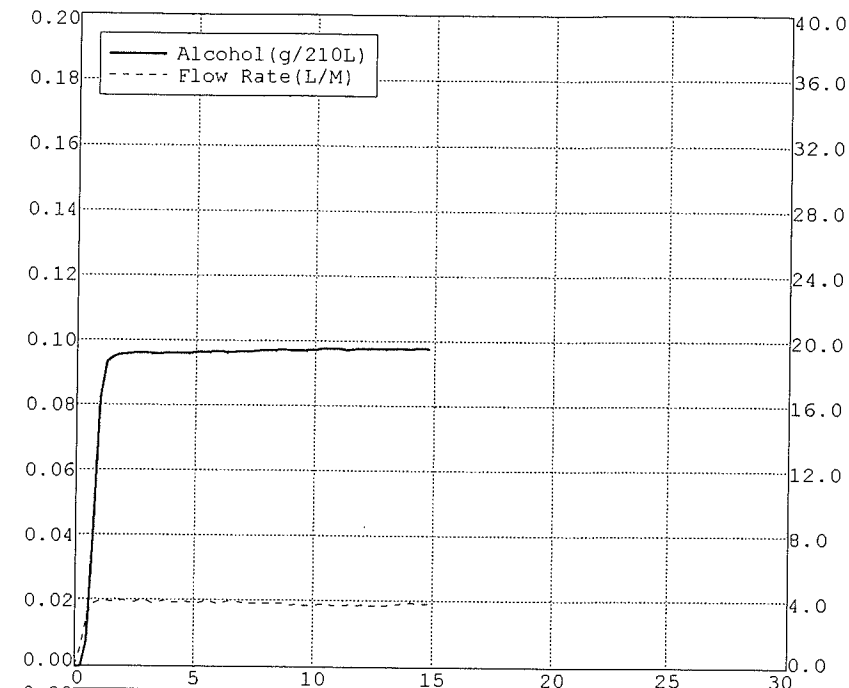

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/23/2024

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:33
INTERNAL STANDARD	VERIFIED	05:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:34
BLANK TEST	0.00	05:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:35
BLANK TEST	0.00	05:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:36
BLANK TEST	0.00	05:37

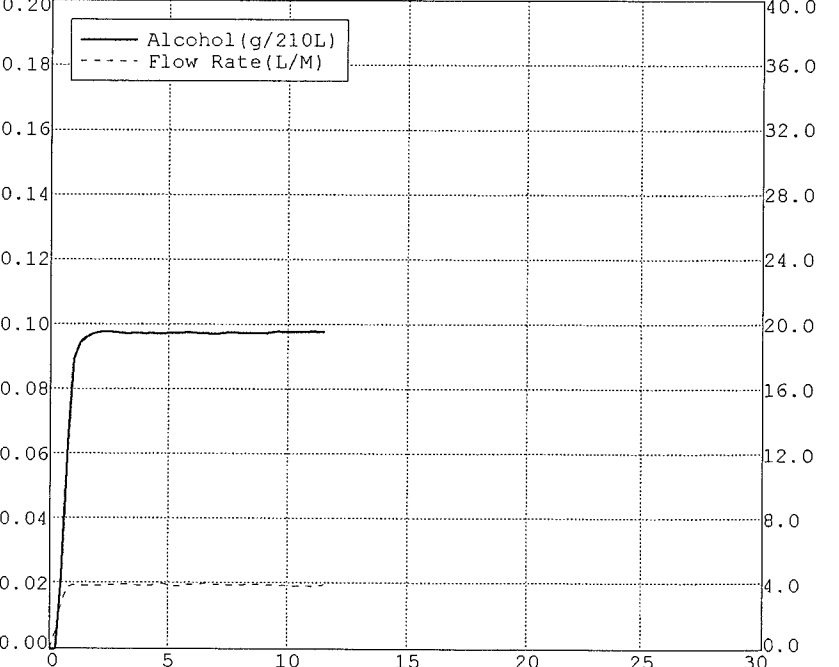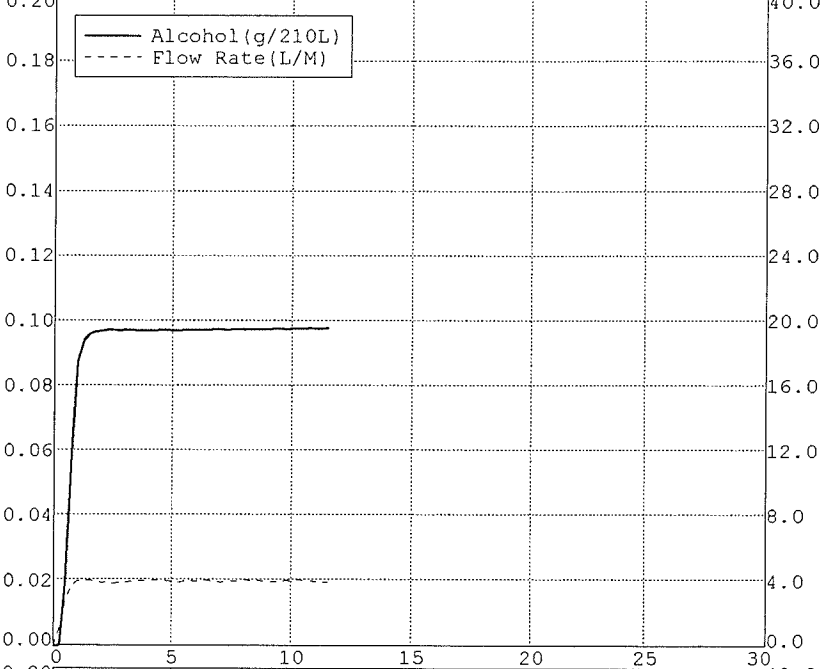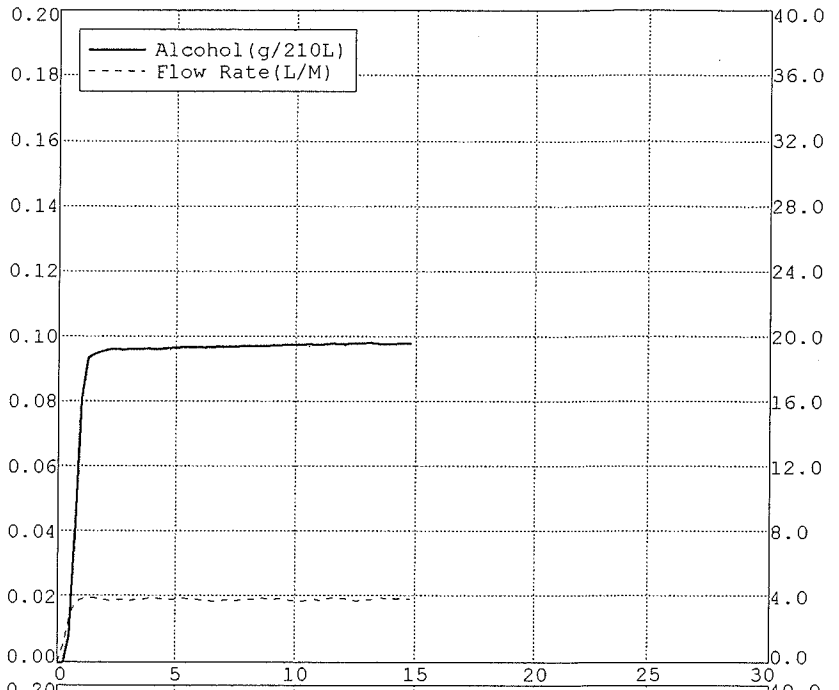

SUPERVISOR TEST

LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/30/2024

OPERATOR NAME:  
MAKENZIE A HAYES  
Permit #: 49532  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 24140

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:14
INTERNAL STANDARD	VERIFIED	18:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:15
BLANK TEST	0.00	18:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:16
BLANK TEST	0.00	18:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:17
BLANK TEST	0.00	18:18

